

TURBOVAC 850 i(X), 950 i(X), 1350 i, 1450 i Turbomolecular Pumps with Integrated Frequency Converter


Operating Instructions 300855170_002_C8

Part Nos.

84007xVxxxx 84008xVxxxx 84009xVxxxx 84010xVxxxx

850092Vxxxx(U) 850102Vxxxx(U) 850122Vxxxx(U) 850132Vxxxx(U)

x = 0 to 9

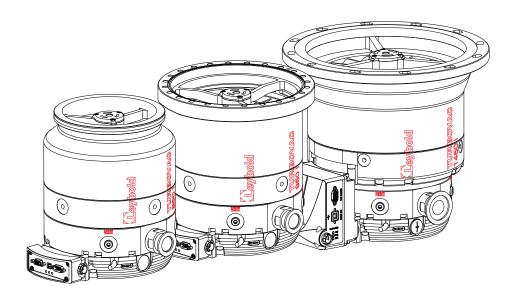

Contents

		Page
0	Important Safety Information	5
	Safety symbols	5
0.1	Mechanical hazards	6
0.2	Electrical hazards	7
0.3	Thermal hazards	7
0.4	Danger through materials and substances	7
0.5	Dangers in connection with safety-related measures and precautions	7
1	Description	8
1.1	Design	10
1.2	Standard equipment	10
1.3	Technical data	11
1.3.1	Technical data for the integrated drive electronics	12
1.3.2	Pumping speed curves	13
1.3.3	Operation diagrams	15
1.4	Ordering data	19
2	Transport and storing	23
2 3	Transport and storing Installation	23 24
_		
3	Installation	24
3 3.1	Installation Conforming utilization	24 24
3 3.1 3.1.1	Installation Conforming utilization Non-conforming utilization	24 24 24
3 3.1 3.1.1 3.2	Installation Conforming utilization Non-conforming utilization Operating environment	24 24 25
3 3.1 3.1.1 3.2 3.3	Installation Conforming utilization Non-conforming utilization Operating environment Fitting accessories	24 24 25 26
3 3.1 3.1.1 3.2 3.3 3.4	Installation Conforming utilization Non-conforming utilization Operating environment Fitting accessories Attach the pump to the vacuum chamber	24 24 25 26 27
3 3.1 3.1.1 3.2 3.3 3.4 3.5	Installation Conforming utilization Non-conforming utilization Operating environment Fitting accessories Attach the pump to the vacuum chamber Forevacuum connection	24 24 25 26 27 35
3 3.1 3.1.1 3.2 3.3 3.4 3.5 3.6	InstallationConforming utilizationNon-conforming utilizationOperating environmentFitting accessoriesAttach the pump to the vacuum chamberForevacuum connectionConnect the cooling	 24 24 25 26 27 35 36
3 3.1 3.1.1 3.2 3.3 3.4 3.5 3.6 3.6.1	Installation Conforming utilization Non-conforming utilization Operating environment Fitting accessories Attach the pump to the vacuum chamber Forevacuum connection Connect the cooling Air cooling	24 24 25 26 27 35 36 36
3 3.1 3.1.1 3.2 3.3 3.4 3.5 3.6 3.6.1 3.6.2	InstallationConforming utilizationNon-conforming utilizationOperating environmentFitting accessoriesAttach the pump to the vacuum chamberForevacuum connectionConnect the coolingAir coolingWater cooling	24 24 25 26 27 35 36 36 37
3 3.1 3.1.1 3.2 3.3 3.4 3.5 3.6 3.6.1 3.6.2 3.6.3	InstallationConforming utilizationNon-conforming utilizationOperating environmentFitting accessoriesAttach the pump to the vacuum chamberForevacuum connectionConnect the coolingAir coolingWater coolingWater quality	 24 24 25 26 27 35 36 36 37 38 40 41
3 3.1 3.1.1 3.2 3.3 3.4 3.5 3.6 3.6.1 3.6.2 3.6.3 3.7 3.8 3.9	InstallationConforming utilizationNon-conforming utilizationOperating environmentFitting accessoriesAttach the pump to the vacuum chamberForevacuum connectionConnect the coolingAir coolingWater coolingWater qualityConnect a power failure venting valve or a venting valveConnect a flange heater	24 24 25 26 27 35 36 36 36 37 38 40 41 42
3 3.1 3.1.1 3.2 3.3 3.4 3.5 3.6 3.6.1 3.6.2 3.6.3 3.7 3.8	InstallationConforming utilizationNon-conforming utilizationOperating environmentFitting accessoriesAttach the pump to the vacuum chamberForevacuum connectionConnect the coolingAir coolingWater coolingWater qualityConnect a power failure venting valve or a venting valveConnect purge gas	 24 24 25 26 27 35 36 36 37 38 40 41

Contents

4	Operation	49
4.1	Media compatibility / purge gas	49
4.2	Interfaces	49
4.3	Switching on	51
4.4	Shutting down	52
4.5	Venting	53
4.6	Bakeout	54
4.7	Operation after a longer storage period	54
4.8	Removing the pump from the system	55
-	Maintenance	EG
5	Maintenance	56
5 5.1	Cleaning	56
5.1	Cleaning	56
5.1 5.2	Cleaning Leybold Service	56 56
5.1 5.2 5.3	Cleaning Leybold Service Bearing monitoring and conditioning	56 56 57
5.1 5.2 5.3 6	Cleaning Leybold Service Bearing monitoring and conditioning Troubleshooting	56 56 57 59

The TURBOVAC allows through both standard and optional interfaces controlling of the pump and setting up of some pump functions according to specific requirements. The Operating Instructions **300450826 Serial Interfaces for TURBOVAC i/iX** offers detailed information on the RS 232, RS 485, Profibus and USB interfaces of the TURBOVAC.

The Operating Instructions **300687441 TURBOVAC iX EtherCAT Interface** offers information on the EtherCAT Interface.

The Operating Instructions **300905828 TURBOVAC i Interface Module** describes the Anybus modules.

These Operating Instructions are a translation of the German original instructions 300855170_001_C8.




Obligation to Provide Information

Before installing and commissioning the pump, carefully read these Operating Instructions and follow the information so as to ensure optimum and safe working right from the start.

The Leybold **TURBOVAC** has been designed for safe and efficient operation when used properly and in accordance with these Operating Instructions. It is the responsibility of the user to carefully read and strictly observe all safety precautions described in this section and throughout the Operating Instructions. The pump must only be operated in the proper condition and under the conditions described in the Operating Instructions. It must be operated and maintained by trained personnel only. Consult local, state, and national agencies regarding specific requirements and regulations. Address any further safety, operation and/or maintenance questions to our nearest office.

"Trained personnel" for the operation of this pump are

- skilled workers with knowledge in the fields of mechanics, electrical engineering and vacuum technology and
- personnel specially trained for the operation of vacuum pumps.



WARNING indicates a potentially hazardous situation which, if not avoided, could result in death or serious injury.

CAUTION indicates a potentially hazardous situation which, if not avoided, could result in minor or moderate injury.

NOTICE is used to notify users of installation, operation, programming or maintenance information that is important, but not hazard related.

We reserve the right to alter the design or any data given in these Operating Instructions. The illustrations are not binding.

Retain the Operating Instructions for further use.

0 Important Safety Information

Safety symbols

The safety symbols on the products shows the areas where care and attention is necessary.

The safety symbols that follow are used on the product or in the product documentation.



0.1 Mechanical hazards



WARNING: EJECTION OF PARTS

If the mounting is not sturdy enough, pump blockage could cause the pump to break loose; internal pump components could be thrown in all directions.

Mount the pump firmly to the vacuum chamber. Never operate the pump without proper flanging to the vacuum chamber (in bench testing, for example).

In case of rotor destruction a sudden twisting of the entire pump is possible. The vacuum chamber must be able to absorb the torque of max. 5 kNm (TURBOVAC 850/950 i) or 9 kNm (TURBOVAC 1350/1450 i) around the rotor's axis of rotation in the event of sudden rotor destruction.



CAUTION: CUTTING AND CRUSHING

When reaching into open flanges there is a risk of cutting and crushing your fingers.

Do not operate the vacuum pump with open flanges. Do not reach into the pump.

When installing the vacuum pump, first mechanically connect the inlets and outlets and then make the electrical connections.

Disconnect the vacuum pump from the power supply before servicing. Only use trained service personnel.

Before servicing, ensure that gas cannot flow through the pump. Only open the pump system when it is under atmospheric pressure.



CAUTION: EJECTION OF PARTS

Ejection of parts through bursting of vacuum system as a result of excessive pressure.

When using the pump with purge gas, protect the purge gas supply such that in the event of a malfunction no overpressure can occur within the system. The pressure in the pump must not exceed 1.4 bar (absolute).



CAUTION: VACUUM

Pulling into the vacuum can cause injury to hands or fingers.

Do not operate the vacuum pump with open flanges.



CAUTION: FALLING PARTS

Errors during transport can cause the pump to fall down.

Transport the pump only in its transport packaging or at the eye-bolts provided for this purpose.

0.2 Electrical hazards



CAUTION: ELECTRICAL SHOCK

Contact with live parts may lead to electrical shock.

The electrical connection may only be carried out by a trained person. Observe the national regulations in the user country, e.g. for Europe EN 50110 - 1. Prior to servicing, disconnect the vacuum pump from the power supply.

Electrical shock due to interruption of the protective conductor system. In the event of a fault, life-threatening voltages may be present on electrically conductive components. Before commissioning, check the resistance of the earthing cable and the suitability of the assigned overcurrent protection device.

The pump must only be connected to power supplies which meet the requirements for functional extra-low voltages with positive isolation in accordance with IEC 60364-4-41 (or local regulations) (PELV). All interfaces must only be operated with PELV-fed components and devices.

0.3 Thermal hazards



CAUTION: BURNS

Touching hot surfaces may lead to burns.

Handle the pump only when ventilated and cooled down. Wear suitable protective equipment.

0.4 Danger through materials and substances

WARNING: HAZARDOUS SUBSTANCES

Pumped process gases may escape from the exhaust and leaks in the vacuum system. During servicing, toxic deposits may be present in the pump. The gases, vapours or substances may be hazardous to health.

The pumping of toxic / explosive / flammable / pyrophoric / radioactive / oxidizing / corrosive gases or gas mixtures, as well as oxygen of more than atmospheric concentration (21 %) is generally prohibited. The operator is responsible for assessing the hazard potential of the process media or mixtures.

0.5 Dangers in connection with safety-related measures and precautions



CAUTION: AUTOMATIC START-UP

The frequency converter is not equipped with its own emergency shut down switch. This may lead to an unwanted pump start-up.

Install an emergency shut down switch in the system. The emergency shut down switch must be present in the building installation

- suitably arranged and easily accessible for the user
- marked as the disconnecting device for this device.

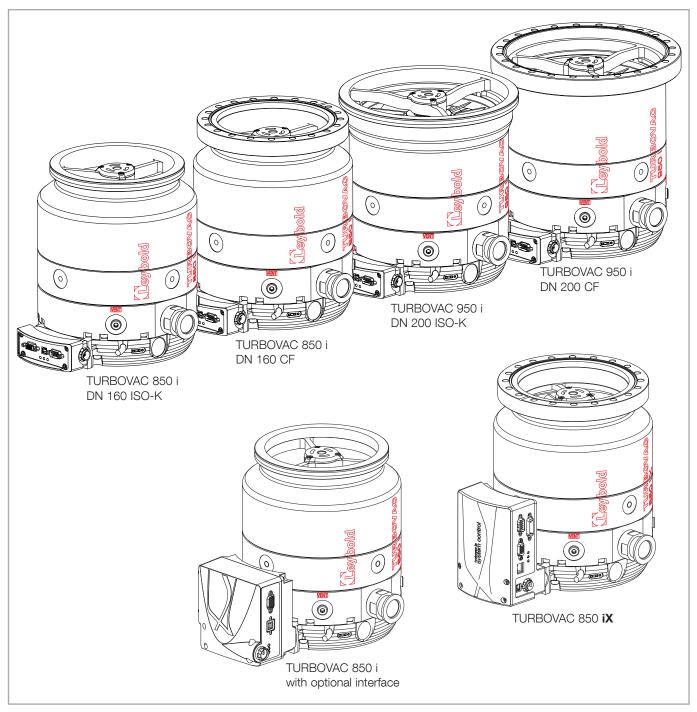


Fig. 1.1 TURBOVAC models

1 Description

The TURBOVAC 850 i(X), 950 i(X), 1350 i and 1450 i are turbomolecular pumps designed to evacuate vacuum chambers down to pressure levels in the high vacuum and ultra-high vacuum range.

They are suitable for pumping air and clean gases. A forevacuum pump and a power supply are required for their operation.

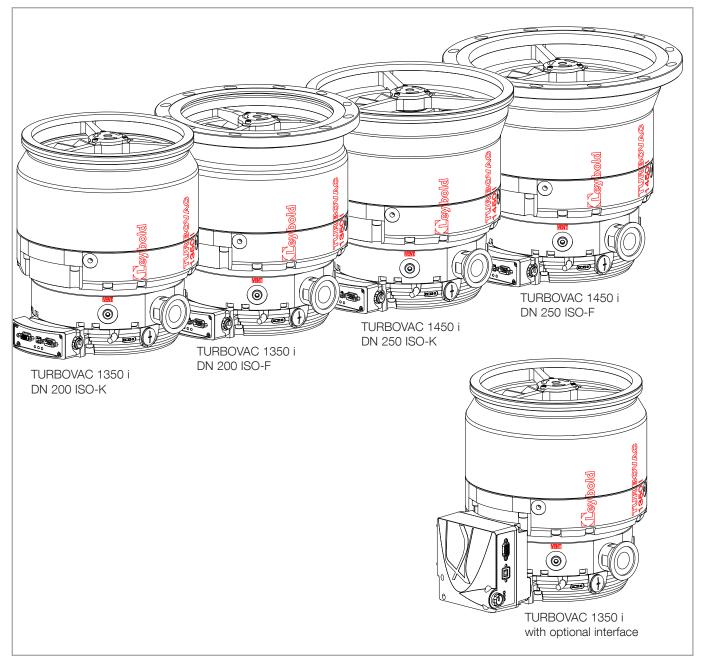


Fig. 1.2 TURBOVAC models

1.1 Design

The TURBOVAC models are wide-range TMPs equipped with an additional Holweck stage.

With the built-in frequency converter as the electronic drive the TURBOVAC forms one single unit. The electonic drive governs the pump's speed and serves as a monitor for all functions of the pump. Moreover, the TURBOVAC **iX** is equipped with an integrated vacuum system controller for connection and operation of various accessory components.

At the high vacuum side the bearing is of a non-wearing permanent magnetic bearing type, at the forevacuum side a lifetime lubricated oil-free ceramic ball bearing is used.

Water cooling or an air cooling fan is available for the TURBOVAC 850 i and 950 i as optional equipment. The TURBOVAC 1350 i and 1450 i are water-cooled as standard.

The intake flange should be fitted with a wire mesh inlet screen to protect the pump against mechanical damage caused by foreign objects.

The pumps are equipped with a venting and a purge gas facility. The connections are blanked off by default with G1/8" closure screws.

Venting and purge gas valves, or a venting screw, or a pressure regulator can be connected directly to the pump.

1.2 Standard equipment

Turbomolecular pump with integrated electronic drive unit, two eye-bolts

High and fore-vacuum flanges are protective-capped.

Flange mounting elements and the inlet screen are not enclosed, but are available as accessories.

1.3 Technical data

1 1 1 > 1 > 1 4 2	250 ISO-K 250 ISO-F 40 KF 1380 1280 1390 1210 24** 2 8 0 10 ⁸ 10 ⁸ 10 ⁸ 10 ⁹ 5.10 ^{.9}		
1250 1150 1350 1150 > 2 1 1 1 1 2.1 2.1	1380 1280 1390 1210 24** 2 8 0 10 ⁸ 10 ⁵ 10 ⁴		
1150 1350 1150 > 2 1 1 1 1 1 2	1280 1390 1210 24** 2 8 0 10 ⁸ 10 ⁶ 10 ⁴		
1 1 2 3 1 2	2 8 0 ·10 ⁸ ·10 ⁸ 10 ⁵ 10 ⁴		
> 1 4. 2.	·10 ⁸ 10 ⁵ 10 ⁴		
< 7.5	5·10 ⁻⁹		
4	4		
42 000	42 000		
23 100	23 100		
2.5	2.5		
00 (default). 800 (max.)	600 (default). 800 (max.)		
50	50		
40 54 1			
+5 bis +40¹) -15 bis +70			
Water	Water		
_	_		
r 6x1 hose / screw-in thre	ead		
60			
6			
5			
	42 000 23 100 2.5 00 (default). 300 (max.) 50 0 ¹⁾ 70 Water - r 6x1 hose / screw-in three		

 * Please contact us when using Argon or other "heavy" gases as process gas.


** For a high gas throughput with $\mathrm{N}_{\!_2}$ please contact Leybold.

1) Depending on the ambient temperature, the gas throughput and the type of gas, forced air cooling or water cooling may be necessary.

	850 i(X)	950 i(X)	1350 i	1450 i
kg	14.6 /	15.4 / – / 21.7	23.5 / 24.3 /	24.4 / 25.5 / _
	ECODRY 65 plus. TRIVAC D 65 B. SCROLLVAC 7 plus. DIVAC 3.8 HV3			
dB(A)	< 40 < 55	< 40 < 55	< 44 _	< 44
°C	100			
	approx. 85% (non-condensing)			
mbar · I · s ⁻¹ sccm	0.4 24			
	G 1/8"			
	G 1/8"			
	dB(A) °C mbar · I · s⁻¹	kg 14.6 / - / 19.6 E SC dB(A) < 40 < 55 °C mbar · I · s ⁻¹	kg $14.6 / - /$ $15.4 / - /$ 19.6 21.7 ECODRY 65 plus SCROLLVAC 7 plus dB(A) < 40	kg $14.6 / - /$ $15.4 / - /$ $23.5 / 24.3 /$ 19.6 21.7 - ECODRY 65 plus. TRIVAC D 65 E SCROLLVAC 7 plus. DIVAC 3.8 HY dB(A) < 40

1.3.1 Technical data for the integrated drive electronics

	TURBOVAC i	TURBOVAC iX
	Drive electronics	Drive electronics and vacuum system control unit
Supply voltage	48 V DC +5 % / -10 %	48 V DC +5 % / -10 %
Max. current consumption	11 A (default), 13 A (max.) at 48 V DC	11 A (default), 13 A (max.) at 48 V DC
Max. power consumption TURBOVAC 850/950 i TURBOVAC 1350/1450 i	500 W (default), 600 W (max.) 600 W (default), 800 W (max.)	500 W (default), 600 W (max.)
Interfaces	see ordering data	see ordering data
Residual ripple	< 3 %	< 3 %
Max. length of the DC cable (for variants with removable front end)	0,5 m	_
Max. contact rating of the relays	48 V, 0.5 A 24 V, 1.0 A	48 V, 0.5 A 24 V, 1.0 A
Overvoltage category	II	II
Contamination grade	2	2
Accessory connections	1 pc. M8 connector, 24 V DC	3 pcs M8 connector, 24 V DC
Maximum load rating for the 24 V DC outputs (powering accessories, e.g. cooling unit or valves)	24 V, max. 18 W	24 V, 12 W
Vacuum gauge head connection	-	15 pin Sub-D

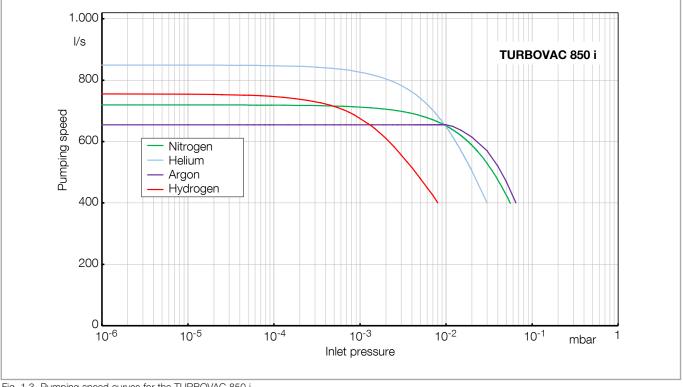

1.3.2 Pumping speed curves

Fig. 1.3 Pumping speed curves for the TURBOVAC 850 $\ensuremath{\mathsf{i}}$

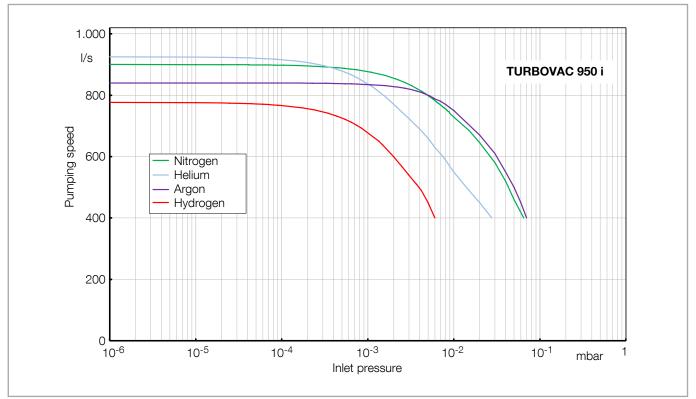


Fig. 1.4 Pumping speed curves for the TURBOVAC 950 i

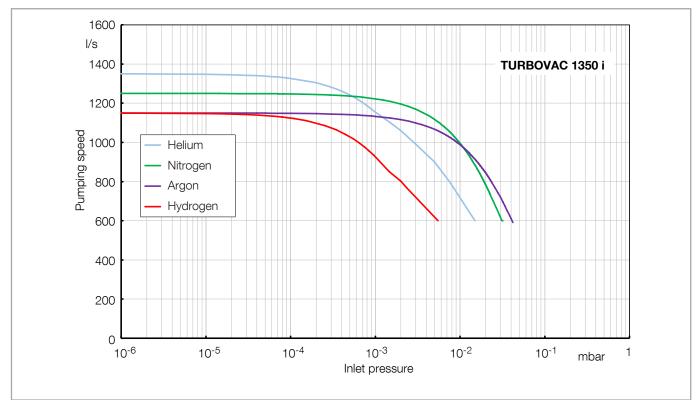


Fig. 1.5 Pumping speed curves for the TURBOVAC 1350 i

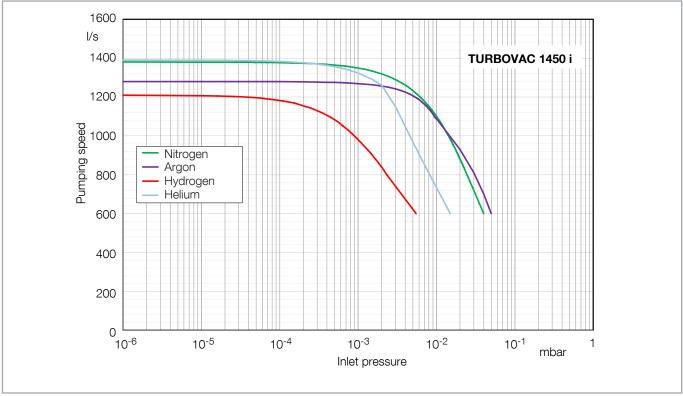


Fig. 1.6 Pumping speed curves for the TURBOVAC 1450 $\ensuremath{\mathsf{i}}$

1.3.3 Operation diagrams How to read the operating diagram for nitrogen for the TURBOVAC 850i:

With deploying a SCROLLVAC 7 plus backing pump gas flows may be transported permanently with maximum throughput quantities of

- 0.2 mbar·l/s (with convection cooling),
- 0.5 mbar·l/s (with air cooling at 40 °C), and
- approx. 5 mbar·l/s (with cooling water at 35 °C).

These values result of the intersection between the limitations of the individual cooling variant and the pumping speed of the backing pump given. As can be seen, maximum permanent gas flows are not solely a TMP characteristic, but are dependent from the installed backing pump, too.

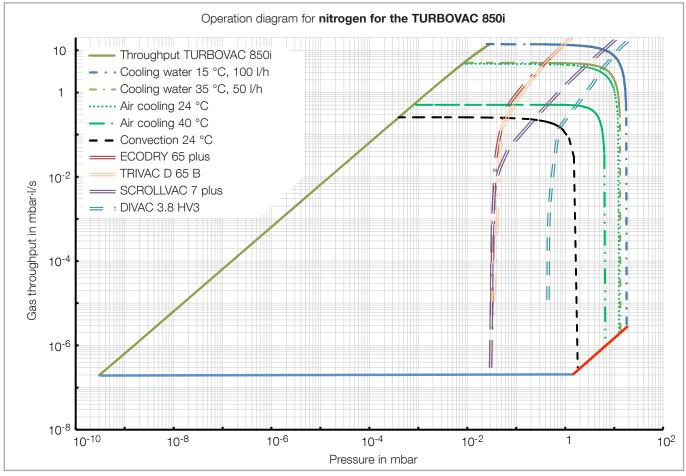


Fig. 1.7 Operation diagram for TURBOVAC 850 i

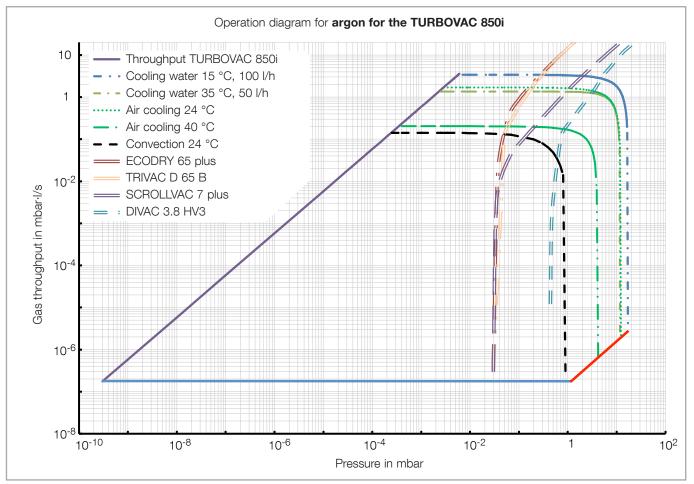


Fig. 1.8 Operation diagram for TURBOVAC 850 i

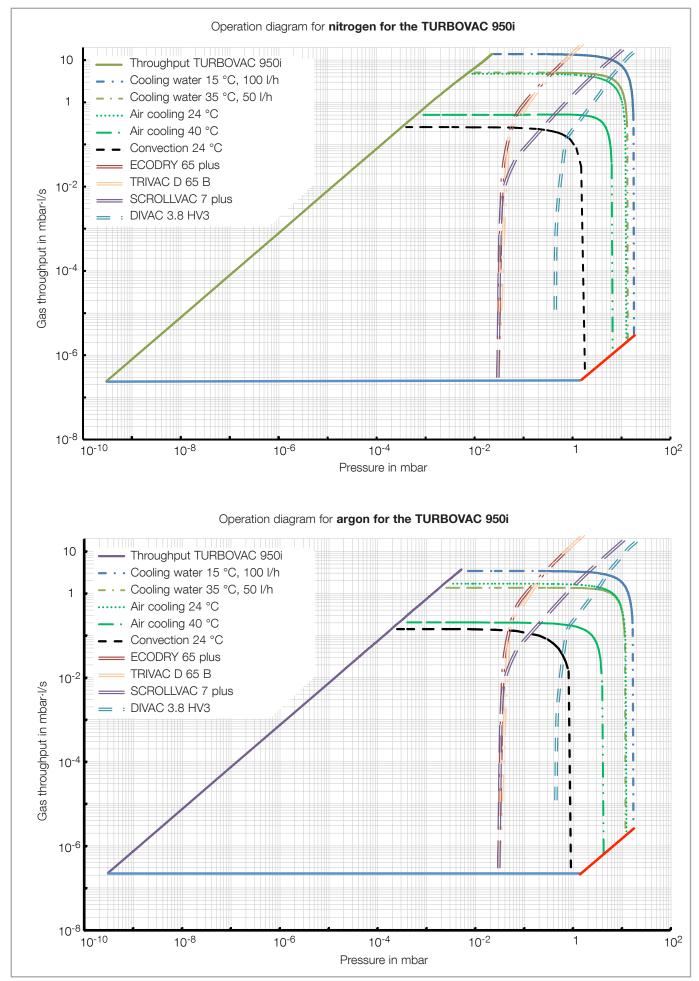


Fig. 1.9 Operation diagrams for TURBOVAC 950 i

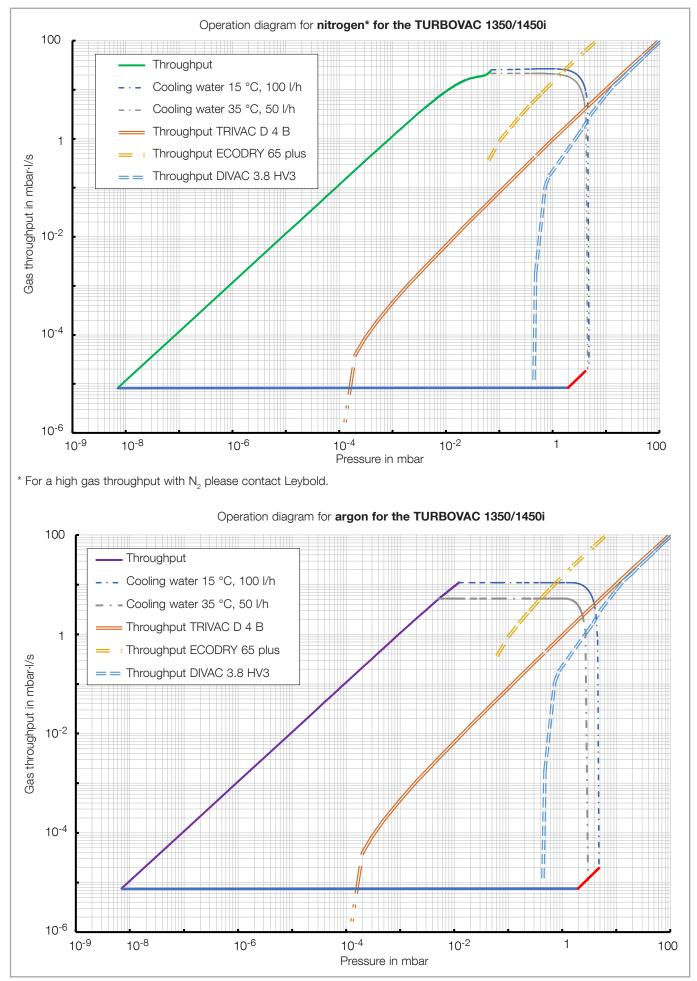


Fig. 1.10 Operation diagrams for TURBOVAC 1350 i and 1450 i

1.4 Ordering data

TURBOVAC	850 i	950 i
RS 485, USB+, 15-pin digital I/O interface		
High-vacuum flange	160 ISO-K	200 ISO-K
Part No. Pump with optional interface	840071V1000 840071V2000	840091V1000 840091V2000
High-vacuum flange	160 CF	200 CF
Part No. Pump with optional interface	840081V1000 840081V2000	840111V1000 840111V2000

Optional interface (RS 232, Profibus, Ethernet/IP, Profinet, EtherCAT), USB+, 15-pin digital I/O interface: on request

TURBOVAC	850 iX	950 iX
TONDOVAO	000 17	330 IX
RS 485, USB+, 15-pin digital I/O interface		
High-vacuum flange	160 ISO-K	200 ISO-K
Part No. Pump with dummy in the Anybus slot Pump with RS 485 in the Anybus slot	840071V3000 840071V3300	840091V3000 840091V3300
High-vacuum flange	160 CF	200 CF
Part No. Pump with dummy in the Anybus slot Pump with RS 485 in the Anybus slot	840081V3000 840081V3300	840111V3000 840111V3300

TURBOVAC	1350 i	1450 i
RS 485, USB+, 15-pin digital I/O interface		
High-vacuum flange	200 ISO-K	250 ISO-K
Part No. Pump with optional interface	850092V1000 850092V1000U 850092V2000 850092V2000U	850122V1000 850122V1000U 850122V2000 850122V2000U
High-vacuum flange	200 ISO-F	250 ISO-F
Part No. Pump with optional interface	850102V1000 850102V1000U 850102V2000 850102V2000U	850132V1000 850132V1000U 850132V2000 850132V2000U

Optional interface (RS 232, Profibus, Ethernet/IP, Profinet, EtherCAT), USB+, 15-pin digital I/O interface: on request

TURBOVAC 850 i and 950 i pumps can be mounted in any orientation.

TURBOVAC 1350 i and 1450 i pumps can be mounted

- horizontally or vertically with the high-vacuum flange on top and in any orientation in between or
- horizontally or vertically with the high-vacuum flange on the bottom and in any orientation in between (U versions)

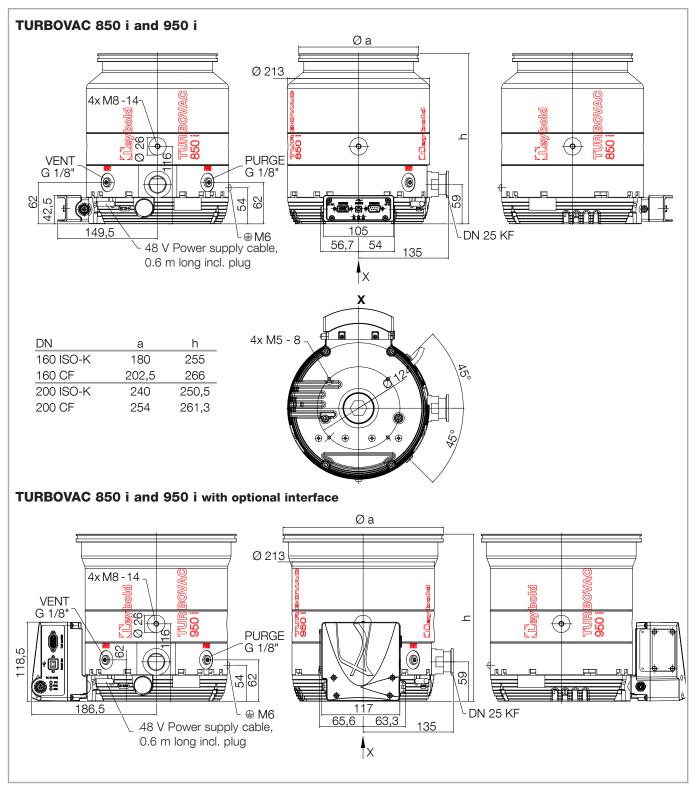


Fig. 1.11 Dimensional drawings, dimensions in mm

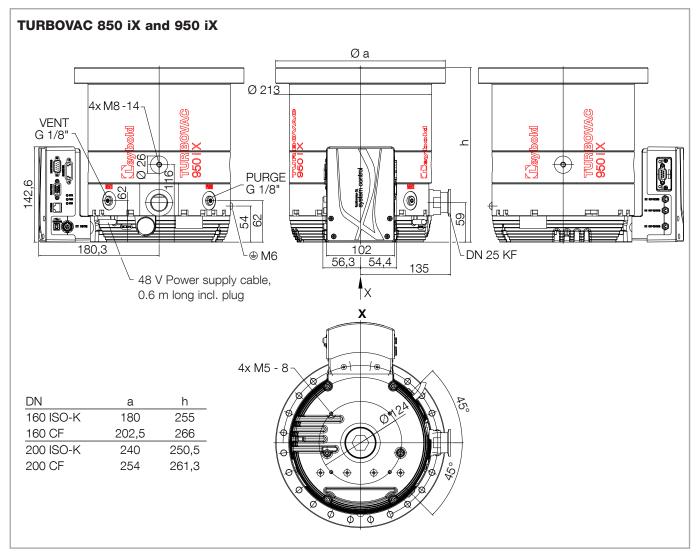


Fig. 1.12 Dimensional drawings, dimensions in mm

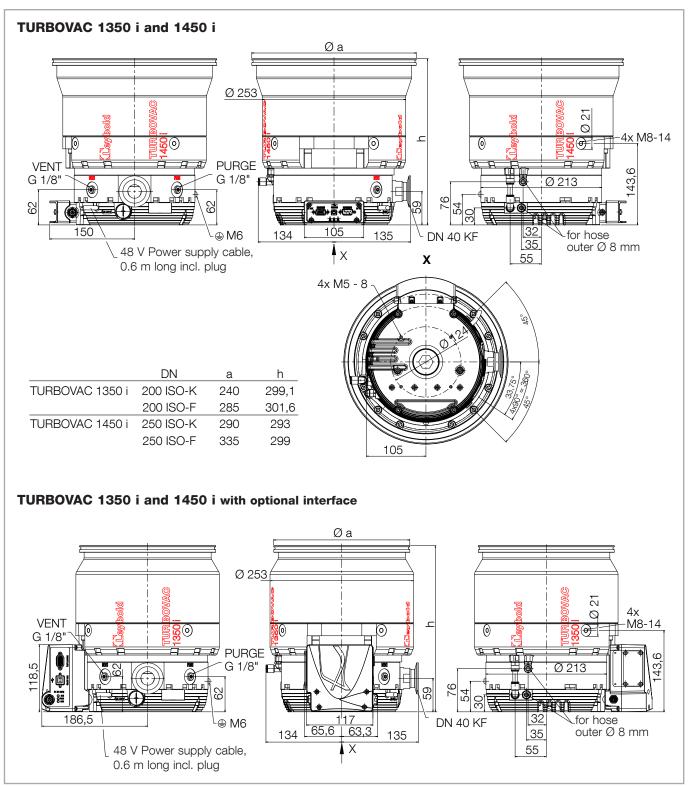


Fig. 1.13 Dimensional drawings, dimensions in mm

Transport and storing

2 Transport and storing

Transport

The devices are delivered in safe transport packaging. Check whether the packaging has been damaged during transport. If that is the case, notify the freight forwarder and Leybold if necessary.

Keep transport packaging for any further transportation and storage of the pump. Be careful not to damage the sockets and connections during handling.

Unpacking

The turbomolecular pump is shipped in a sealed PE bag with desiccant. Do not open the PE bag until immediately before installing. Do not remove the covers and blanking flanges until you are ready to make the connections, to ensure that the turbomolecular pump is installed under the cleanest possible conditions.

The pump is equipped with four M8 boreholes for eye-bolts for transport. Remove the pump from the packaging using the two eye-bolts provided, guiding it with one hand.

Transport the pump only in its transport packaging or at the eye-bolts provided for this purpose. Do not stand below the pump while connecting or removing the turbomolecular pump.



Storing

To store the devices, place them in a sealable PE bag containing a drying agent and use the supplied transport packaging. Do not store pump and accessories in a moist atmosphere so as to prevent these items from suffering corrosion. Take note of details in Section 4.8.

For pumps that have been stored for more than 12 months, a ball bearing run-in procedure must be carried out before operation, see Section 4.7.

For pumps that have been stored for more than 3 years, we recommend a preventive exchange of the ball bearings, see Section 5 Bearing replacement.

3 Installation

3.1 Conforming utilization

The turbomolecular pump is intended for generating a vacuum. It is suited for non-corrosive processes only.

The turbomolecular pump must be bolted to a rigid vacuum system and connected to a suitable backing pump.

It is intended for being operated within closed rooms.

The use of any accessories which have not been specified by Leybold is only allowed after approval by Leybold.

3.1.1 Non-conforming utilization

Non-conforming utilizations for both pump and frequency converter are among others:

- Pumping of gases and vapours for which the materials of the pump are unsuitable.
- Operation in connection with processes in which GaAs (gallium arsenide) is being pumped.
- Pumping of gas mixtures with an oxygen content of > 21%.
- Pumping of corrosive gases and dust containing gases without reverting to purge gas operation.
- Pumping of condensable vapours without suitably controlling the temperature of the pump. Upon compression within the pump, these vapours may condense or form deposits.
- Pumping of dusts and solids without the use of suitable screens and filters.
- Operation at an inadmissibly high forevacuum pressure.
- Operation at inadmissibily high gas loads.
- Utilization of both pump and frequency converter in explosion hazard areas.
- Non-compliance of the specified maintenance and servicing intervals
- Operation of the pump and drive electronics in environments which demand a higher protection type than that of the pump and where the installation site is over 4000 m the above sea level.
- Utilization in systems and pump systems in which the pressure may exceed 1.4 bar abs.
- Operation with an inadequately mounted pump
- Operation without having flanged the pump to the system or without having connected it to a suitable backing pump.
- Operation with additional heat sources involving thermal radiation, thermal conduction via the high vacuum or the forevacuum flange, strong magnetic fields or very hot process gases, for example. In environments with water cooling operation, CF flanges may be baked-out up to 100 °C.

- Use in systems in which impact stress and vibrations or periodically occurring forces affect pump, frequency converter and cables.
- Operation on moving system or system components (locks, for example).
- Operation at vibration absorbers and vacuum components (gate valves, valves) which are not capable of sustaining the specified deceleration torque should the pump rotor seize.
- Stepping on pump, add-on parts, drive electronics, flanges and cables to climb onto the system.
- Fitting of add-on parts to the forevacuum flange which cause an inadmissible high load.
- Removing, covering or obstructing warning notices.
- Standstill or storing of the pump without suitable sealing-off and drying. Storing in a humid atmosphere can cause corrosion.
- Conversions, manipulations and maintenance work by personnel not authorised by Leybold..

Any non-conforming utilisation of pump, frequency converter and accessories can result in severe injury or death and cause damage to components.



3.2 Operating environment

Permissible ambient tem-	5 to 40 °C
perature	Depending on the ambient temperature, the gas throughput and the type of gas, forced air cooling or water cooling may be necessary.
	no dripping or spraying water (for pumps with IP40), no explosive gas atmospheres
Installation altitude	up to 4000 m
	At altitudes over 2000 m heat dissipation by the ambi- ent air is impaired.

3.3 Fitting accessories

Only for TURBOVAC i

Secondary devices are directly energised and activated via the accessory connection X201 (M8 plug); by means of a Y-cable 2 accessories can be connected at the same time.

In this case both devices will be switched parallelly (i.e. de-energised active / in-active). The factory-set accessories's interface features a plug-and-play mode, and is instantly ready for operation with the connected device (energised with pump switched on).

Only for TURBOVAC iX

Additional accessory components can be connected to the TUBOVAC iX

- Pressure gauge
- Further 24 V DC operated equipment which may be driven depending on the pump status.

The accessory components can be electrically powered and driven through three accessory connections. The following table shows the TURBOVAC iX configuration as delivered from the factory:

Accessory connec- tion	Pre-configured equipment	Reaction
X201	Air cooling	Air cooling unit is running when the TURBOVAC is running.
X202	Relay box for fore- vacuum pump	Forevacuum pump is running when the TURBOVAC has received the start command.
X203	Venting valve	The venting valve opens when the start com- mand is revoked and the frequency drops below 999 Hz. At 5 Hz the valve is closed again (no power failure venting!).



Fig. 3.1 Mounting position

3.4 Attach the pump to the vacuum chamber

Mounting position

TURBOVAC 850 i and 950 i pumps can be mounted in any orientation. TURBOVAC 1350 i and 1450 i pumps can be mounted

- horizontally or vertically with the high-vacuum flange on top and in any orientation in between or
- horizontally or vertically with the high-vacuum flange on the bottom and in any orientation in between (U versions)

The pump can be damaged if it is operated if it is operated in the incorrectly installed position. Observe the sticker on the pump and install the pump only in the permitted orientation.

Never touch the rotor. Touching the rotor may cause injury and damage the rotor bearing.

If the mounting is not sturdy enough, pump blockage could cause the pump to break loose; internal pump components could be thrown in all directions.

Mount the pump firmly to the vacuum chamber. Never operate the pump without proper flanging to the vacuum chamber (in bench testing, for example).

Do not operate the vacuum pump with open flanges. Do not reach into the pump.



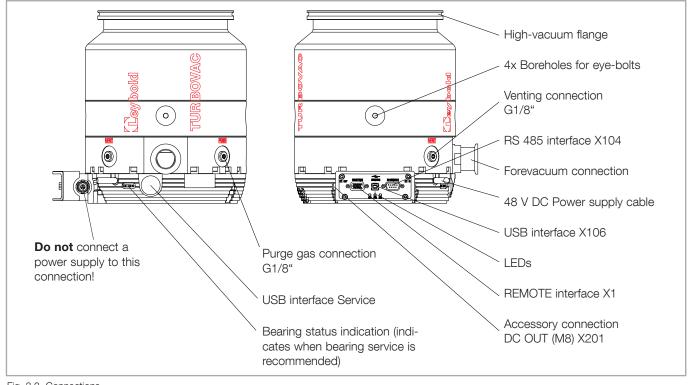


Fig. 3.2 Connections

Remove the transport seal from the intake flange and remove the desiccant. Pay attention to maximum cleanliness when connecting.

Torque when the rotor seizes

In the case of a sudden rotor vane rupture or rotor-stator contact which may occur in practice (caused, for example, by solid objects from the process chamber entering the pump through the high vacuum flange), the following torques need to be absorbed by the system:

TURBOVAC 850/950 i(X)	max. 5 kNm
TURBOVAC 1350/1450 i	max. 9 kNm

In most applications the pump is flanged to the high vacuum flange at the apparatus. The pump can be mounted and operated in any desired attitude.

When using flange connecting elements in accordance with DIN 28404 (ISO-F flange connection), ISO 1609 (ISO-K flange connection) or ISO 3669 (CF flange connection), which fit positively to the pump flange, check the maximum load capacity of the connecting element. Not all flange components can withstand the forces that occur in a crash.

If the strength of the component is not sufficient, there is the possibility of providing an additional safeguard via the four threaded holes for the eye-bolts for transport. Ensure that the mountings can withstand the braking torque.

The flange material to which the pump is bolted, must have at operating temperature a minimum strength specification of 150 N/mm².

If several turbomolecular pumps are installed to the vacuum chamber of the same system, there is the risk of interference (vibration interference between the pumps). If such a risk exists please contact Leybold Application Support.

The standard mounting arrangement for the pump is adequate to ensure earthquake protection. If required mount the system to the floor or the walls.

Install a splinter guard or an inlet screen

To protect the TMP against foreign material from the vacuum vessel we recommend to mount a centering ring with a fine or coarse inlet screen at the high vacuum flange, though this will reduce the pumping speed at the chamber flange.

Reduction of the pumping speed in %		Не	N ₂	Ar
Fine inlet screen DN 160/200/250	6	9	20	23
Coarse inlet screen DN 160/200/250	1	2	6	7

Damages caused during operation without the inlet screen are excluded from warranty.

Flange mounting for ISO-K flanges

When flanging on the high vacuum connecting flange, place the O-ring on the centering ring. The O-ring must remain in place smooth and untwisted. Thereafter put the outer ring (support ring) in place.

Mount the turbomolecular pump according to Fig. 3.3 and 3.4 and tighten the bolts crosswise step-by-step.

When using an ultra sealing ring, always use an outer support ring. The information on the number of bolts and clamps also applies to the ultra sealing rings.

Required for the installation:

- mounting kit (accessories)
- coarse or fine inlet screens (accessories, optional)

The contact surfaces of pump housing, vacuum system and centering ring must be free of grease and dry so as to ensure adequate strength in case the rotor should seize.



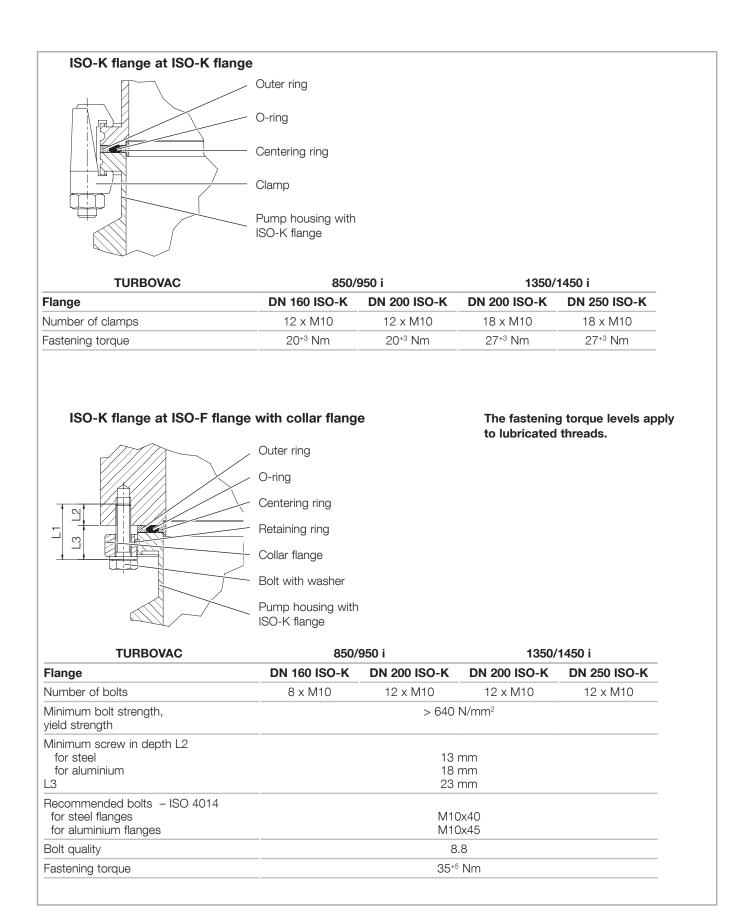


Fig. 3.3 Mounting high vacuum flange ISO-K


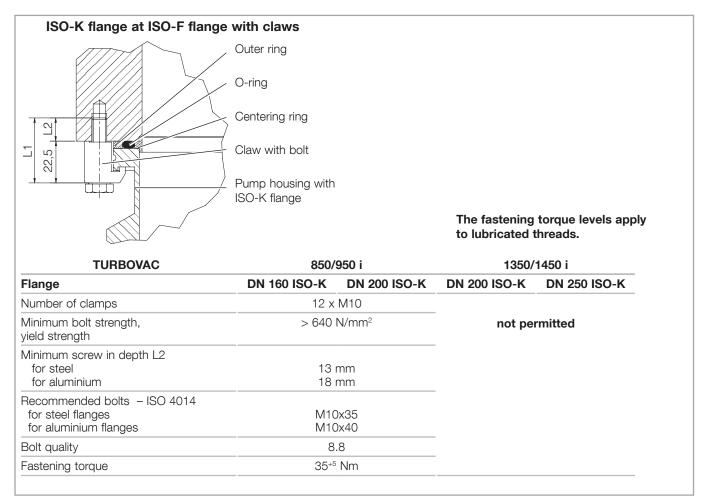


Fig. 3.4 Mounting high vacuum flange ISO-K

Flange mounting for CF flanges

Before fitting, check to ensure that the sealing edge is undamaged. Do not touch the copper gasket and the sealing edge with your bare hands.



Mount the turbomolecular pump according to Fig 3.5 and tighten the bolts step-by-step.

When the pump shall be baked out, the threads of the bolts should have been lubricated with a high temperature lubricant.

Required for the installation:

- mounting kit (accessories)
- coarse or fine inlet screens (accessories, optional)



NOTICE

During operation the pump can get so hot that there is the risk of suffering burns (up to approximately 65 °C). Protect the hot parts against being touched.

Flange mounting for ISO-F flanges

Mount the turbomolecular pump according to Fig 3.6 and tighten the bolts crosswise step-by-step.



The contact surfaces of pump housing, vacuum system and centering ring must be free of grease and dry so as to ensure adequate strength in case the rotor should seize.

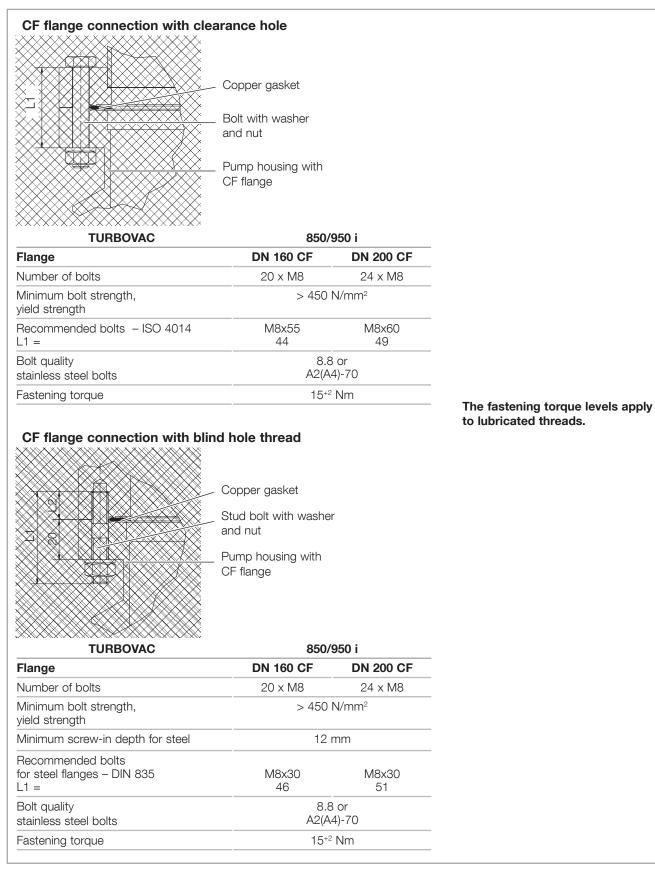


Fig. 3.5 Mounting the CF high vacuum flange

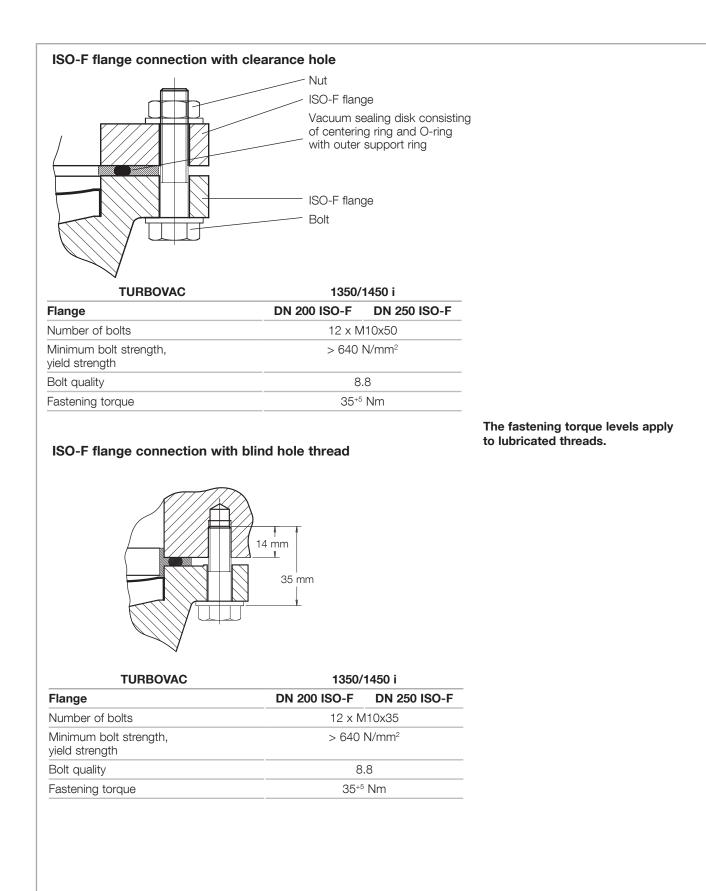


Fig. 3.6 Mounting the ISO-F high vacuum flange

3.5 Forevacuum connection

Connect the clean forevacuum line with the small flange connectors and take care not to constrict the forevacuum flange's diameter.

Ensure that the pump is sufficiently isolated against vibrations generated by the forevacuum pump.

No forces from the piping system may be allowed to affect the turbomolecular pump. Support the piping correspondingly or decouple through flexible joints.

Do not use the pump with a backing pressure below 5×10^{-4} mbar. Lower backing pressures will increase the evaporation rate of the lubrication reducing the bearing life.

The forevacuum line must be tight. Hazardous gases can escape at leaks or the gases being pumped can react with air or humidity. Observe Safety Information 0.4.

Only for TURBOVAC i

The forevacuum pump can be energised at the accessories connection of the TURBOVAC via the relay box.

Only for TURBOVAC iX

A forevacuum pump may be electrically connected through the relay box to accessory connection X202 on the TURBOVAC iX.

The relay box switches the forevacuum pump on when a start command is present for the turbomolecular pump, and the relay box switches the forevacuum pump off when the start command is revoked.

Through parameter 643[1] the switch-on delay time and through parameter 644[1] a shutdown delay time in seconds can be set up (the default for both parameters is 0).



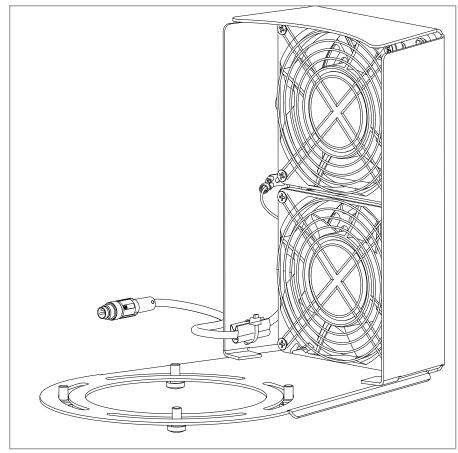


Fig. 3.7 Air cooling

3.6 Connect the cooling

Cooling of the pump depends on the required pumping power and the ambient temperature. When the pump is insufficiently cooled it will shut down.

High gas throughputs, cyclic operation or high ambient temperatures will necessitate air or water cooling.

3.6.1 Air cooling

When installing air cooled pumps within a system ensure that sufficient quantities of fresh air are freely available. The air cooling facility is powered via the pump.

Use the 4 bolts which are included in the delivery to attach the air cooling unit at the bores provided on TURBOVAC. Plug in the control cable of the air cooler into the accessories connection and screw tightly. The accessory connection is so pre-configured that the air cooler will always be running when the pump is running. To change this setting, refer to the interface Operating Instructions.

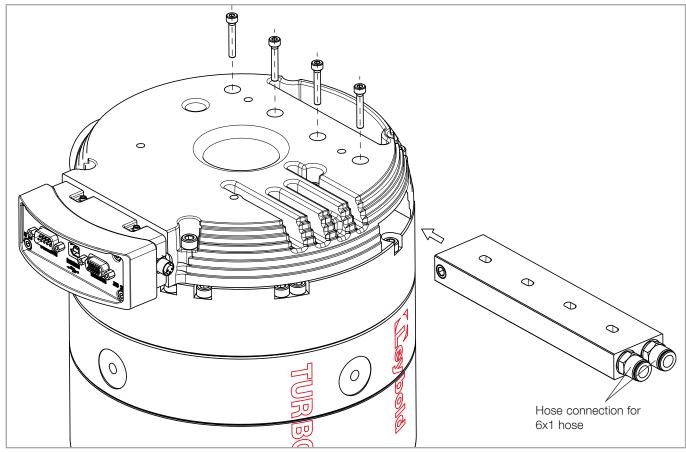


Fig. 3.8 Attaching the water cooling to the TURBOVAC 850 i and 950 i

3.6.2 Water cooling

TURBOVAC 850 i and 950 i

Attach the cooling water block to the TURBOVAC with 4 M4 screws, tightening torque is 3^{+1} Nm. Connect the cooling water hoses.

TURBOVAC 1350 i und 1450 i

The TURBOVAC have water cooling as standard. Insert the cooling water hoses, see Fig. 3.9.

The hose connections may be unscrewed and removed, to make use of the integrated G 1/8"-threads.

Adjust the cooling water temperature so that the formation of condensate is avoided. With pump downtimes the cooling water has to be turned off.

When switching the cooling water supply on and off by means of an electrically actuated valve, connect the valve so that it will be switched on and off together with the pump.

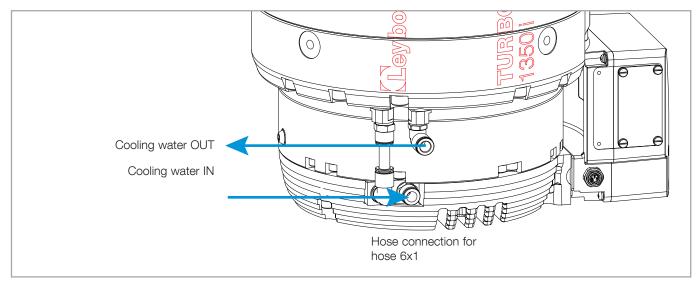


Fig. 3.9 Connect the water cooling to the TURBOVAC 1350 i and 1450 i

3.6.3 Water quality

In order to ensure long trouble-free operation the cooling water must not contain any oils, greases and suspended solids. Moreover, we recommend compliance with the following limit values:

Appearance	Clear, free of oils and greases
Suspended matter	< 250 mg/l
Particle size	< 150 μm
Electrical conductivity	< 700 µS/cm
pH value	7.0 to 9.0
Total hardness (total alkaline earths)	< 8 °dH
Aggressive carbon dioxide	None, not detectable
Chloride	< 100 mg/l
Sulphates	< 150 mg/l
Nitrate	≤ 50 mg/l
Iron	< 0.2 mg/l
Manganese	< 0.1 mg/l
Ammonium	< 1.0 mg/l
Free chlorine	< 0.2 mg/l
9°dU (degrees Cormon bardness) 1 (122201/l

8 °dH (degrees German hardness) = 1.4mmol/l

= 10 °e (degrees English hardness)

= 14 °f (degrees French hardness)

If there is the danger of frost, you may use a water glycol mixture of up to 30 %.

DS water (softened or fully desalinated water) can be used for cooling the pump, if the pH value corresponds to the range indicated above.

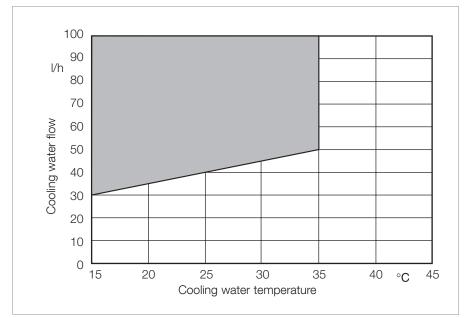


Fig. 3.10 Cooling water requirements

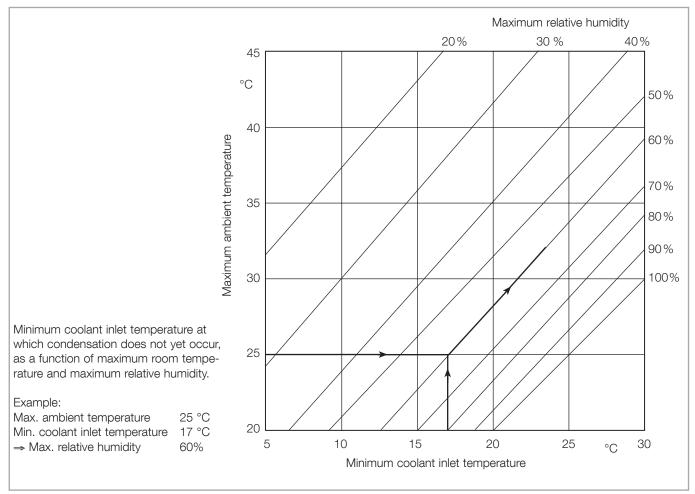


Abb. 3.11 Dewpoint diagram

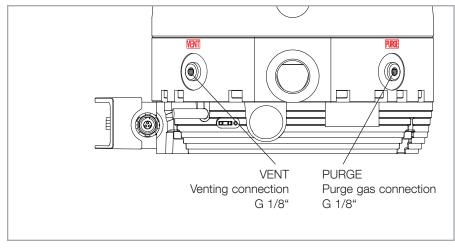


Fig. 3.12 Venting and purge gas connections

3.7 Connect a power failure venting valve or a venting valve

The power failure venting valve (normally open) or venting valve (normally closed) vents the pump and the forevacuum line when the pump is switched off and thus keeps oil vapor from diffusing back from the forevacuum line. A choke nozzle in the vent port ensures that the pump is not vented too fast.

The max. permissible pressure in the pump must not exceed 1.4 bar (abs.).

Unscrew and remove the locking screw and the gasket from the venting connection of the TURBOVAC.

Screw in the venting valve and the gasket into the venting connection. To protect the threads, the max. fastening torque is 5 Nm.

If applicable connect the venting gas supply at the valve's inlet (G1/8").



When using the pump with purge gas, protect the purge gas supply such that in the event of a malfunction no overpressure can occur within the system. The pressure in the pump must not exceed 1400 mbar (0.4 bar overpressure).





Connect a purge gas or venting valve to the correct flange. Confusing the venting and purge gas flange can cause shock venting of the pump.

Only for TURBOVAC i

Plug in the corresponding control cable into the accessories connection.

For the electronic drive unit change the venting valve settings to venting operation (via the interfaces).

Only for TURBOVAC iX

Plug in the corresponding control cable into the accessories connection X203. Accessory connection X203 is so pre-configured that the venting valve opens when the start command is revoked and the frequency drops below 999 Hz. At 5 Hz this valve is closed again. This is no power failure venting! The limits can be changed through parameter 28[2] (upper switching thresh-

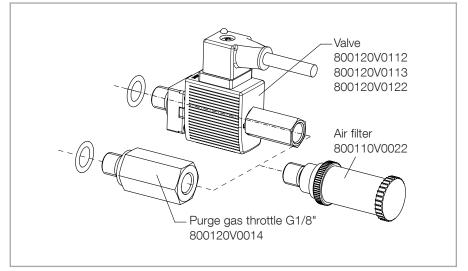


Fig. 3.13 Fitting valve

old) and parameter 647[2] (lower switching threshold). For this refer to the interface Operating Instructions.

Either connect a power failure venting valve electrically separately or connect it to X201, X202 or X203 and thereafter change the function for the accessory connection. For this refer to the interface Operating Instructions.

3.8 Connect purge gas

When having to decide which gases need or not need to be pumped with purge gas we are available to provide assistance.

Refer to Section 4.1 for suited gases.

Consider the additional purge gas flow when selecting a suitable backing pump.

We recommend a purge gas flow of 0.4 mbar·l/s (24 sccm) with Nitrogen.

The pressure in the pump must not exceed 1400 mbar (0.4 bar over- pressure).



The purge gas is fed either through an activated valve or a manually operated throttle.

Purge gas connection with purge gas valve

Unscrew and remove the locking screw and the gasket from the purge gas connection of the TURBOVAC.

Screw in the purge gas valve and the gasket into the thread.

Connect the purge gas supply at the valve's inlet (G1/8").

Either connect the purge gas valve electrically separately or connect it to an accessory connection and thereafter change the function for the accessory connection. For this refer to the interface Operating Instructions.

Purge gas connection with purge gas throttle

Unscrew and remove the locking screw and the gasket from the purge gas connection of the pump.

Then screw in the throttle and the gasket into the thread.

3.9 Connect a flange heater

Only for TURBOVACs with CF flange

If pressures in the range of 10⁻⁸ mbar or below are to be developed, the vacuum chamber and the components installed therein will have to be baked out. In addition, the TURBOVAC can be baked out using the flange heater provided for this purpose.

With the aid of the relay box the heating jacket can be driven directly via the turbopump. For this connect the heating jacket to the relay box and insert the connection cable of the relay box at the accessory connection (X201 for the TURBOVAC iX) and screw it down.

The accessory connection has been so pre-configured that the heating jacket will heat as long as the turbomolecular pump is running. To change this setting, refer to the interface Operating Instructions.

Alternatively the heating jacket may be connected through the corresponding mains power cable to the power supply.

Information on baking out is also given in Section 4.6.

3.10 Connect a vacuum gauge head (only for TURBOVAC iX)

One of the listed vacuum gauge heads may be connected to connection X101.

Connect the vacuum gauge head only after having switched off the pump first.

Vacuum gauge head	Connection cable	Pressure range
TTR 101, TTR 101 S2, TTR 101 N, TTR 101 N(S2)	Type F	5 x 10 ⁻⁴ 1500 mbar
ITR 200 S, ITR 200 SL, ITR 200 SP, ITR 200 SD	Туре С	5 x 10 ⁻¹⁰ 1000 mbar
CTR 100/101, CTR 100 N, CTR 101 N	Туре С	1 x 10 ⁻¹ 1000 torr to 1 x 10 ⁻⁵ 0,1 torr
TTR 91, TTR 91 S, TTR 96 S, TTR 91 N, TTR 91 N(S), TTR 96 N(S)	Туре F	5 x 10 ⁻⁴ 1000 mbar
PTR 90, PTR 90 N	Type F	5 x 10 ⁻⁹ 1000 mbar
ITR 90, ITR 90 P	Туре С	5 x 10 ⁻¹⁰ 1000 mbar

The type of connected vacuum gauge head is detected automatically.

The measured value can be read out in millibar, Torr and Pascal through parameter as real value.

P616: measured value in millibar P617: measured value in Torr P618: measured value in Pascal

Further parameters (like filter time, CTR vacuum gauge head subtype, gas type correction factor etc., for example) may be set up for the respective vacuum gauge head.

For this refer to the interface Operating Instructions.



3.11 Electrical connection

Observe Safety Information 0.2

Unplug any connectors only when the mains voltage is switched off **and** the pump does no longer turn.

The frequency converter is not equipped with its own emergency shut down switch. This may lead to an unwanted pump start-up.

Install an emergency shut down switch in the system. The emergency shut down switch must be

- present in the building installation
- suitably arranged and easily accessible for the user
- marked as the disconnecting device for this device.

The pump can be operated with 48 V DC power supply. Take note of the performance data specified in Section 1.3.1.



Fig. 3.14 Power supply connector

The cable protection and voltage drop and the minimum supply voltage must be adhered to when wiring.

When operating more than one pump with a single power supply, it may be necessary to fuse each pump separately due to the line protection.

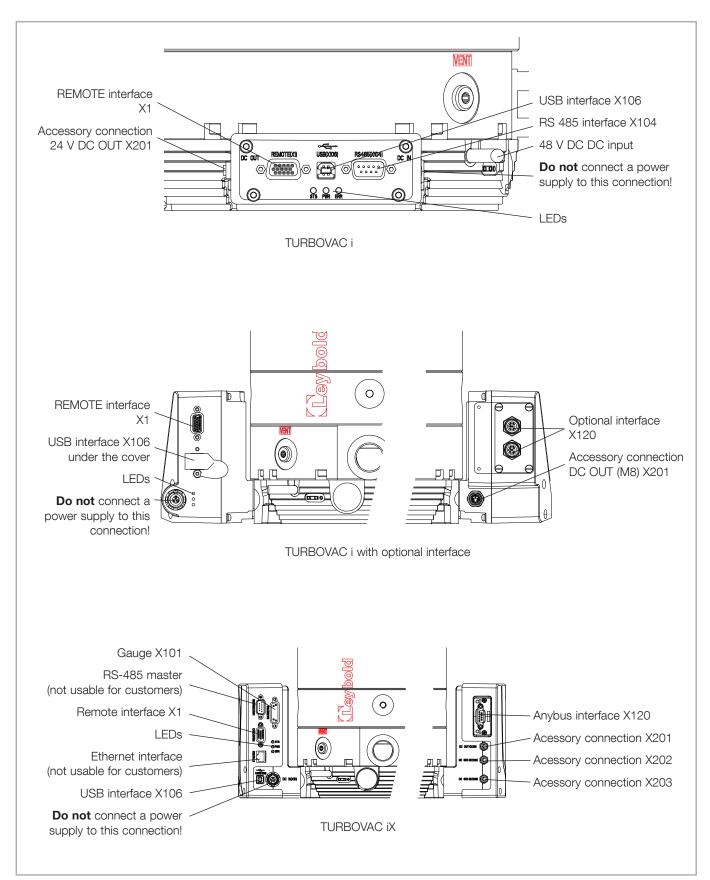



Fig. 3.15 Interfaces

STS PWR	green LED STATUS off: flashes slowly 1/s: flashes fast 3/s: flashes slowly 0.5/s: on:	Pump at standstill (< 3 Hz) Start command is present (about Running up Running down Normal operation	10 s after start)
err err	yellow LED POWER off: flashes 1/s: flashes 3/s: on:	No supply voltage Supply voltage too low or too high Running down and pump speed < Supply voltage is present	
	red LED ERROR off: flashes: on:	No error, no warning Warning is present, pump can be or run-in procedure is running Fault is present, pump stopped or	operated possibly with some restrictions
	Possible reasons: Initialisation shortly a 	hich it cannot be controlled fter switching on the supply voltage n progress (power supply must not b ing is ongoing	e interrupted) Valid from firmware parameter P2: R02.09.01

Fig. 3.16 LEDs


Earth (ground) connection

We recommend fitting a separate earth (ground) conductor. The impedance between the pump body and the earth connection point must be < 0.1 $\Omega.$

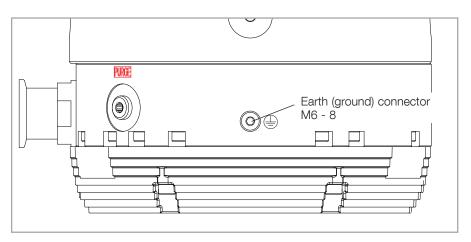

REMOTE X1

15-pole Sub-D female



Maintain pin 6 Signal GND and pin 13 Analog GND separate so as to avoid equalisation currents.

Pin	Name	Description
1	Error relay	(com)
2	Error relay	(n.c.)
3	Normal operation relay	(n.o.)
4	Normal operation relay	(com)
5	Normal operation relay	(n.c.)
6	Signal GND	
7	High level output	24 V, 100 mA, Tolerance acc. to device supply voltage
8	Start input (High) Reset input (Low)	High > 10 V ± 0,5 V Low < 7.5 V ± 0,5 V
9	Error relay	(n.o.)
10	Standby input	High > 10 V ± 0.5 V Low < 7.5 V ± 0.5 V
11	Cooling/Venting valve input (Low)	High > 10 V ± 0.5 V Low < 7.5 V ± 0.5 V
12	Analog output (Default: Frequency)	0 10 V, 2 mA
13	Analog GND	
14	Warning relay	(n.c.)
15	Warning relay	(com)
Shield	Connected with pump housing	

Start/Stop input

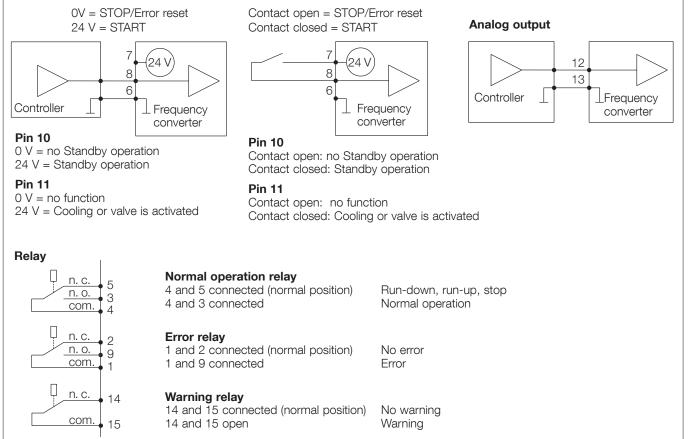


Fig. 3.17 REMOTE interface X1

Relay status

Input	data / s	status			Outpu	t data			Operating mode
Start/ stop signal	Pump rotating	Normal frequency ≥ 90% of setpoint frequency	Error is present		Relay NORMAL DPERATION	Relay ERROR	LED STATUS (green)	LED ERROR (red)	Other modes are not possible; they indicate a failure affecting the frequency converter.
Stop	no	no	no	off	passive	passive	off	off	Pump not operating
Stop	yes	no	no	off	passive	passive	flashes	off	Pump is decelerating
Stop	yes	yes	no	off	passive	passive	flashes	off	Just after stop; pump was in the normal operating mode before that
Start	no	no	no	on	passive	passive	off	off	Just after start
Start	yes	no	no	on	passive	passive	flashes	off	Pump is accelerating
Start	yes	yes	no	on	active	passive	green	off	Pump is in the normal operating mode
Stop	no	no	yes	off	passive	active	off	red	Error is present; pump is at standstill
Stop	yes	no	yes	off	passive	active	flashes	red	Error is present; pump is decelerating
Stop	yes	yes	yes	off	passive	active	flashes	red	Error has just occurred
Start	no	no	yes	off	passive	active	off	red	Error is present; pump is at standstill
Start	yes	no	yes	off	passive	active	flashes	red	Error is present; pump is decelerating
Start	yes	yes	yes	off	passive	active	flashes	red	Error has just occurred

4.1 Media compatibility / purge gas

The TURBOVAC integra is suitable for pumping air and clean gases.

If reactive gases in low concentrations must be pumped operate the pump with purge gas.

We would be glad to consult with you as regards the media which can safely be handled with this unit.

Install a micropore filter when pumping media which contains dust.

Suited for venting or purging are all gases,

- which will not cause corrosion or pitting in aluminium and steel and
- which in connection with process deposits in the pump will not cause corrosion or sticking.

For venting and as the purge gas we recommend inert gases like nitrogen or argon. The temperature of these gases should be between 5 °C and 80 °C, max. relative humidity should not exceed 10 ppm.

The gas must be clean.

In individual cases and after consultation also dry, filtered, oil-free air or filtered ambient air may be used (filter mesh $<1\mu m$).

Change the filters after some time, at least annually.

4.2 Interfaces

The TURBOVAC i(X) is always equipped with the following interfaces for customers:

USB (COM port) (X106)

■ REMOTE (X1)

Moreover, some models are equipped with an Anybus interface which in turn may be equipped with different interfaces like a RS 485, for example.

The control hierarchy is as follows: Anybus interface \rightarrow USB \rightarrow REMOTE (X1). See also parameter 179.

The frequency converter is configured through the parameters according to the parameter list. Pxxx denotes parameter value xxx.

The PC software **LEYASSIST** can be used for the configuration of the pump and accessories and for data logging. The tool is available for download free of charge on our website.

www.leybold.com \rightarrow Media \rightarrow Downloads \rightarrow Download Software \rightarrow PC Software for Turbomolecular Pumps

Operating Instructions 300450826 Serial Interfaces for TURBOVAC i/IX offer a detailed description of the interfaces RS 232, RS 485, Profibus and USB of the TURBOVAC.

Applications which can be implemented with the aid of the serial interface:

Application	Benefits to the customer	How to do it
Networking of several pumps and other equipment	Savings relating to the costs for sig- nalling cables	With Field Bus systems
Automation	Savings related to repetitive manual work	For example by a control computer
Avoidance of warnings and warnings before overload	Precise planning for maintenance	Monitoring of: Motor current P5
operation and early detection of a failing pump	Improved reliability of sensitive pro- duction processes in a vacuum	 Motor current P3 Motor temperature P7 Frequency converter temperature P11
Standby operation	Cutting process gas consumption	Reducing the rotor's frequency through P24
	Cutting energy consumption	
Troubleshooting	Quick analysis of problems	Reading of error memories P171, P174 and P176: error code, speed, operating hours for error
		Read out warning messages through P227
Slow pressure control by changing the pumping speed	Dispensing with a flow controller	Changing the rotor frequency through parameter 24
Starting the pump with a delay if several consumers are connected to the same PSU	Cost savings through smaller power supply units if peak loads can be reduced	With P36, delay
Lowering the normal opera- tion threshold	Normal operating mode is attained faster, processes can be started faster	Reduce frequency threshold through P25
Only for TURBOVAC iX: Switch the fan depending on temperature or frequency	Saving of electricity, reduce noise, optimise the pump temperature for the process	Configure accessory connection (X201, for example) cor- respondingly, for example, enter function code 30 in parameter 134[0] and set up the temperature limits in parameter 122[0] and 26[0].
Only for TURBOVAC iX: Individually adapt venting and purge gas (active venting, adaptation of the delay time etc.)	Save gas, process speed-up	Correspondingly configure the function code for an accessory connection (X203, for example)
Control cooling water flow	Avoid condensation during cooling water operation	Connect cooling water valve at accessory connection (X201, for example)
Enable generator operation	The power produced by the pump	With P249
(power backup mode)	when running in the generator mode may be used for other electrical con- sumers and the pump is also decele- rated faster.	This function is only changed after de-energising the pump and then restarting it.
Only for TURBOVAC iX: Changing the function of the accessory outputs	Different applications for connected accessories	Configure the accessory connection, see interface Operating Instructions

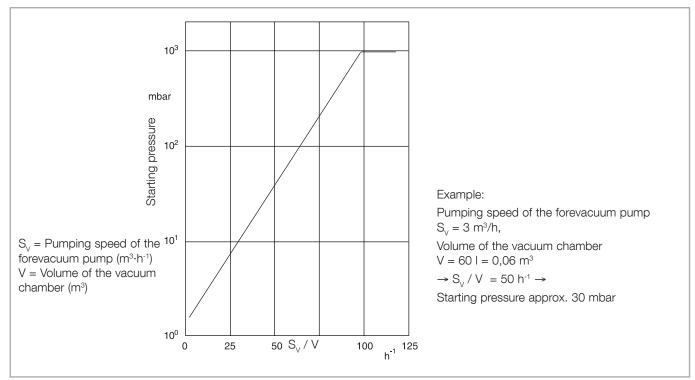


Fig. 4.1 Determining the starting pressure of a turbomolecular pump when evacuating large volumes

4.3 Switching on

For pumps that have been stored for more than 12 months, please take note of Section 4.7.

Switch on the power supply. All LEDs come on one after the other (sequential light), drive electronics (and vacuum system controller) are running up (for approximately 35 seconds).

The maximum starting pressure for the turbomolecular pump can be read from the graph in Fig. 4.1.

Switch on the turbomolecular pump

- via pins 7 and 8 of the socket REMOTE (X1) (For example via a remote control or with the aid of the plug with integrated ON/OFF switch.
- by a start command via the interface.

The turbomolecular pump accelerates. The green LED flashes. When the pump reaches normal operation the green LED lights up permanently.

Avoid the influences of shock and vibration when the pump is running.

Exposure of the pump to accelerating forces must be avoided or reduced to such an extent that the rotor unit will not be excited by vibrations. In the case of critical applications you must consult our Applications Dept. first.

After a mains power failure the pump can run up automatically once more if a start command is present.

Starting pressure




4.4 Shutting down

Switch off the pump.

- via contacts 7 and 8 of the socket REMOTE (X1)
- apply a stop command via the interface
- for the power supply units offered or recommended by Leybold switch off the DC voltage.

After switching off, the green status LED will flash until the rotor of the turbomolecular pump is at standstill. This may take several minutes. With the DC **Generator operation** power supply off, the turbomolecular pump will act as a generator supplying the frequency converter and the control unit with the connected devices with energy as indicated by the yellow power LED. When the generator mode is enabled, the turbomolecular pump supplies power back in to the DC power grid. Switch off the forevacuum pump. Ventina When using oil-sealed forevacuum pumps, vent the turbomolecular pump before it comes to a stop; refer to Section 4.5. When using TRIVAC pumps the built-in anti-suckback valve will close automatically, shutting off the forevacuum line. In forevacuum pumps without a vacuum retention valve, close the valve in the forevacuum line. When the system is not operating, ensure that neither ambient air nor cleaning media can enter the pump. If a failure occurs the turbomolecular pump will be shut down automatically. The red LED at the frequency converter lights up. Under vacuum conditions the pump may take up to one hour to run down, when venting to atmospheric pressure it may take up to one minute. During the time the pump is running down, the green LED will flash, indicating that the rotor has not yet arrived at standstill. When shutting down by switching off the power supply voltage, there will be only enough power for the LEDs down to a speed of the pump of approximately 200 Hz. Thus the pump may still turn without a LED being on. For this reason, when switching off without venting, wait for approximately 15 minutes after the LEDs have turned off until the pump has arrived at standstill. CAUTION Unplug any connectors only when the mains voltage is switched off and the pump does no longer turn.



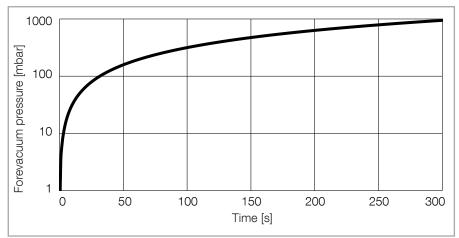


Fig. 4.2 Maximum rise in pressure

4.5 Venting

Refer to Section 4.1 for suited gases.

Venting Methods

There are three different methods of venting the turbomolecular pump.

The pump can be vented via the **venting connection** (VENT), by means of a venting valve, a power failure venting valve, or a venting screw.

Cautious venting of the pump is possible from the **high vacuum side**, since here the bearing forces will be lowest. When doing so, no free jet of gas must be allowed to form on the rotor so as to avoid exposing the rotor to additional forces.

When venting the pump through its **foreline connection**, neither oil nor particles may be entrained in the gas flow from the forevacuum side into the pump.

Speed of the Pressure Rise

All turbomolecular pumps may be vented at full speed. However, the pressure must not increase faster than specified through the pressure rise curve , see Fig. 4.2..

The pump must be vented significantly slower when there is the risk of particles entering into the pump from the process. During venting, the flow must be of the laminar type in both the vacuum chamber and the turbomolecular pump.

The pump must not be vented to pressures above atmospheric pressure.

Speed

Pressure rise curve

Particles

4.6 Bakeout

Only for TURBOVACs with CF flange, see also Section 3.9.

If pressures in the range of 10⁻⁸ mbar or below are to be developed, the vacuum chamber and the components installed therein will have to be baked out. In addition, the TURBOVAC can be baked out using the flange heater provided for this purpose.

Protect the rotor against intensive, direct heat radiation. When baking out at the forevacuum side – at a sorption trap, for example – ensure that the components attached direct are not heated to more than 100 $^{\circ}$ C (212 $^{\circ}$ F).

Operate the pump with water cooling when baking out.

4.7 Operation after a longer storage period



For pumps that have been **stored for more than 12 months**, a ball bearing run-in procedure for smooth ball bearing running must be carried out when putting into operation again. The procedure differs according to the firmware version of the pump, see the following sections.

To do this, set parameter P119 [0] to the value 1 using a serial interface and save the parameter change with parameter P8. Then start the pump.

This process takes approx. 4.3 hours, the red LED will flash during this time. The TURBOVAC may be operated only with low gas throughput during this time.

At the end, the pump accelerates to the nominal speed and parameter P 119 [0] is written to 0 by the electronics.

For pumps that have been **stored for more than 3 years**, we recommend a preventive exchange of the ball bearings, see Section 5 Bearing replacement.

4.8 Removing the pump from the system

Shut down the pump and vent as described in Sections 4.4 and 4.5.

If the pump has previously handled hazardous gases, implement the proper precautionary measures before opening the intake or exhaust connection.

Observe Safety Information 0.4.6.

Disconnect the pump only when it has come to a full stop. The green LED must have gone out.

During run down the pump may still turn without a LED being on, observe the information on emergency shut down given in Section 4.4.

Then switch the mains power off and wait until the yellow power LED is off. Then only disconnect any cable connections.

The pumps may be contaminated with process gases. These gases may be toxic and hazardous to health. In addition, deposits with similarly dangerous properties may have formed. Many of these gases and deposits form acids when they come into contact with humid air. This will result in serious corrosion damage to the pump.

To avoid health hazards and corrosion damage when the pumps are detached from the system, fasten a container of desiccant under the transport cover of the high vacuum connection and then close the pump immediately at all flange connections. Store the pump, with a desiccant, in an airtight PE bag.

Corrosion damage due to faulty packing will nullify the guarantee.

Pack the pump so that it cannot be damaged during shipping and storage. Pay particular attention to protection for the flanges and the electrical plug.

Observe the instructions in Section 5.2 if you forward the pump to Leybold.



Hazardous gases Deposits

Desiccant

Maintenance

Bearing replacement	5 Maintenance We recommend an exchange of the ceramic ball bearings at the fore-vac- uum side after 35,000 operating hours.
	The ceramic ball bearings can be exchanged, if necessary, by our customer service, the nearest Leybold Service Center or by the customer: please contact us for this.
	If you wish to exchange the bearings yourself, you will need a Leybold tool kit and spare ball bearings. Immediately after exchanging the bearings, let them run in, see Section 4.7.
	We recommend an exchange of the rotor unit after 80,000 operating hours at the latest.
	Such maintenance work can only be done by the Leybold Service. If required contact the Leybold service center nearest to your location. You can find the address on our internet page www.leybold.com.
	At high pump loads - for example during cyclic operation, at high gas throughputs or at high ambient temperatures - the aforementioned mainte- nance works should be carried forward. Please consult Leybold for recom- mendations.
Purge gas filter	Depending on the degree of contamination of the purge gas used the filter will clog and will have to be exchanged (our experience indicates that this will become necessary after 1 to 6 months).
Adsorption trap	When an adsorption trap is used, regenerate or renew the adsorption agent regularly; refer to the operating instructions provided with the trap.
	5.1 Cleaning If required clean the turbomolecular pump of dust with a dry cloth.
	Cleaning the frequency converter internally The converter essentially requires no servicing since it contains no compo- nents which could be adjusted.

5.2 Leybold Service

Whenever you send us in equipment, indicate whether the equipment is contaminated or is free of substances which could pose a health hazard. If it is contaminated, specify exactly which substances are involved. You must use the form we have prepared for this purpose.

This form is available from www.leybold.com -> Downloads -> Download Documents.

Provide the form signed by an authorized person for each pump.

This statement detailing the type of contamination is required to satisfy legal requirements and for the protection of our employees.

We must return to the sender any equipment which is not accompanied by a contamination statement.

5.3 Bearing monitoring and conditioning

To ensure maximum reliability and bearing life the TURBOVAC have an integrated system to manage the bearing condition. The status is indicated by a blue LED on the pump.

The pumps have an integrated battery-backed real time clock that is constantly monitoring pump storage time.

If the pump is stored without being run for more than 12 months, "Bearing Run in Mode" (BRIM) is triggered the next time the pump is started to condition the bearing.

If the pump is stored without being run for more than 3 years, the pump will indicate a bearing change is required before the pump is run.

Bearing on-site maintenance

The bearing of the TURBOVAC can be serviced on-site.

Instructions for bearing replacement can be found at https://manuals.leybold. com/en/manual-frontend/products under the part no. of the bearing exchange tool kit.

The following service tool kits and service parts are available.

TURBOVAC	850/950i	1350/1450i
Bearing kit part no.	EK6529255	EK6529260
Bearing exchange tooling part no.	EK850950	EK13501450

Bearing run in mode

Bearing run in mode (BRIM) is a start-up sequence for the pump designed to precondition the bearing to optimise bearing life. The pump goes through a number of speed steps before reaching full speed.

The BRIM process last around 4.3 hours and the LED indicates when this is running.

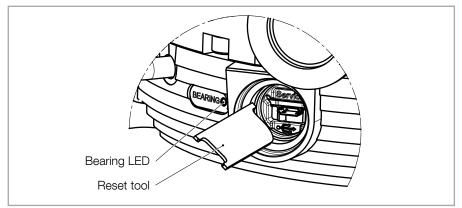


Fig. 5.1 Use the reset tool

Maintenance

Do NOT cancel the BRIM process. This may invalidate the warranty.

BRIM mode is either triggered:

- automatically by the pump
- LeyAssist software
- by pressing the push button (located behind the service cover, see Fig. 5.1) for 2s on the pump, or
- by changing parameter 119 via a serial interface, refer to Operating Instructions 300450826 Serial Interfaces for TURBOVAC i/iX.

Bearing LED

LED is not lit while pump is powered on	No bearing conditioning required
LED is flashing 0.25 s ON and 0.75 s OFF	Pump has been stored for more than 12 months, BRIM is required and will start on the next pump start
LED is permanently ON	BRIM is running
LED is flashing 0.25 s ON and 0.25 s OFF	Pump has been stored for more than 3 years, bearing replacement is required

Troubleshooting

6 Troubleshooting

When the connector cable is attached, the outputs at the frequency converter are not free of voltage.

Before you start searching for the source of the problem, you should carry out a few simple checks:

Are the connections in good working order?

- Mains connection,
- 48 V DC cable to the frequency converter.

Observe the polarity.

Is the forevacuum pressure sufficient?

After having removed the cause for the error reset the error message: By applying a STOP signal via the socket REMOTE (X1), or by a reset sequence via the serial interface or by switching the mains power off.

The error codes can only be read if a serial interface is present.

The following table has been provided as a guide when determining the causes of errors.

Malfunction	Possible cause	Remedy	Shut down
Yellow power LED is not	No DC power	Check cables and power supply	_
on	DC power miswired	Ensure correct polarity of the DC cable.	
	Frequency converter defective	Have the pump repaired. The following may damage the freq. converter: - Disconnection of the DC cable while the pump was still rotating - Non-compliance with the note related to con- necting several pump to a single power supply.	
Red LED flashes	Warning message.	The pump can continue to run, as long as opera- tion limits are only exceeded for a short time. In case of longer exceeding send pump and fre- quency converter to the Leybold service.	no
Turbomolecular pump does not start, ERROR LED does not light.	Interface protocol error	Use USS protocol.	_
	No communication via the serial inter- face.	Connect bus as shown in the interface instruc- tions	
	REMOTE connector (X1) connected wrongly.	Observe Fig. 3.17.	
Turbomolecular pump	Rotor out of balance	Balance the rotor	no
produces loud running noises and vibrations.	Bearing defective	Replace the bearing	



Troubleshooting

Malfunction	Possible cause	Remedy	Shut down
Pump overload, pump cannot keep up its speed.	Forevacuum pressure too high.	Check the ultimate pressure of the backing pump and install a bigger backing pump if req.	yes
When the speed drops	Gas flow too high	Seal leak, check process	
below approx. 90%* of the nominal speed the red	Fan defective	Replace fan	
LED flashes. When this continues for more than 12 min* the pump shuts down.	Water cooling switched off	Switch on water cooling	
Turbomolecular pump	Measurement instrument defective	Inspect the measurement sensor	no
does not reach ultimate oressure.	Measurement sensors soiled	Clean or replace the sensors	
pressure.	Leaks at the equipment, lines or the pump	Check for leaks	
	Pump soiled	Clean the pump	
	Forevacuum pump provides insuffi- cient pumping speed or ultimate pressure which is too high.	Check the ultimate pressure of the forevacuum pump and install a higher-capacity vacuum pump if necessary	
	Frequency parameters programmed wrongly	Check parameters.	
Running pump can not be stopped via X1	Pump has been started via the serial interface, the interface controls the pump	Disconnect the DC supply or connect serial interface and stop via bus	no
Connected accessories do not operate as intended	Accessories incorrectly connected or w wrong function code has been set up or function code dependent parameters have not been properly set up.	Check the settings for the function codes and the corresponding parameters OR check to ensure that the accessories have been connect- ed to the correct accessory connection.	no

60 300855170_002_C8 - 08/2021 - © Leybold

7 Waste Disposal

The equipment may have been contaminated by the process or by environmental influences. In this case the equipment must be decontaminated in accordance with the relevant regulations. We offer this service at fixed prices.

Contaminated parts can be detrimental to health and environment. Before beginning with any work, first find out whether any parts are contaminated. Adhere to the relevant regulations and take the necessary precautions when handling contaminated parts.

Separate clean components according to their materials, and dispose of these accordingly. We offer this service. Further details are available on request.

When sending us any equipment, observe the regulations given in Section "5.2 Leybold service".



Certificates

Certificates

The TURBOVAC i have been tested by the TÜV Rheinland of North America according to the requirements of

UL 61010-1:2012 CSA C22.2 No. 61010-1-12

cTUVus Certificate No. CU 72191742.02

The components are in compliance to the tested standards.

The TÜV Rheinland of North America is a "Nationally Recognized Testing Laboratory" (**NRTL**) for the USA and Canada.



Leybold

EU Declaration of Conformity

Leybold GmbH Bonner Strasse 498 D-50968 Koln Germany Documentation Officer T: +49(0) 221 347 0 documentation@leybold.com

The product specified and listed below

• Turbomolecular Pumps with Integrated Frequency Converter

Type Designation	Part Numbers	Description
<pre> < 3 inlets TURBOVAC a1 a2 a3 i f1 f2 TURBOVAC a1 a2 a3 iX f1 f2 TURBOVAC a1 a2 a3 iC f1 f2 a1 = 850 or 950 or 1350 or 1450, a2 = 10 to 1000, a3 = 1 to 500 (Indices a2 and a3 optional) f1 = 100 to 250 f2 = ISO-K or ISO-F or CF </pre>	8xxxxxVxxxxy x = 0 to 9 y = blank or U	a1 = Pumping speed (first Inlet) a2 = Pumping speed (second Inlet) a3 = Pumping speed (third Inlet) f1 = High Vacuum flange f2 = Flange type i = Communication electronic Frontend or Frontend Anybus iX = Communication electronic Extension box U = Upside Down iC / C = Cartridge - Housing for Customer Application m = Customer-Variants Multi-Inlet
> 3 Inlets TURBOVAC numeral m i TURBOVAC numeral m iC numeral = quad, penta, hexa, hepta, octa, nona, deca (according to the number of inlets) m = 1 to 99	8xxxxxVxxxxy x = 0 to 9 y = blank or C	

Is in conformity with the relevant requirements of European CE legislation:

2006/42/EC Machinery directive Note: The safety objectives of the Low Voltage Directive 2014/35/EU were complied with in accordance with Annex 1 No. 1.5.1 of this directive. 2014/30/EU Electromagnetic compatibility (EMC) directive Class B Emissions, Industrial Immunity 2011/65/EU Restriction of certain hazardous substances (RoHS) directive as amended by Delegated Directive (EU) 2015/863 Based on the relevant requirements of harmonised standards: EN 1012-2:1996 +A1:2009 Compressors and vacuum pumps. Safety requirements. Vacuum pumps EN 61010-1:2010/A1:2019 Safety requirements for electrical equipment for measurement, control and laboratory use. General requirements EN 61326-1:2013 Electrical equipment for measurement, control and laboratory use. EMC requirements. General requirements

This declaration, based on the requirements of the listed Directives and EN ISO/IEC 17050-1, covers all product serial numbers from this date on: 2021-06-14

You must retain the signed legal declaration for future reference

This declaration becomes invalid if modifications are made to the product without prior agreement.

Ian Keech – VP Engineering, Scientific Vacuum Division Burgess Hill

Axel Guddas – General Manager Cologne

Leybold

Declaration of Conformity

Leybold GmbH Bonner Strasse 498 D-50968 Koln Germany

Documentation Officer Innovation Drive Burgess Hill West Sussex RH15 9TW documentation@leybold.com

This declaration of conformity is issued under the sole responsibility of the manufacturer. Turbomolecular Pumps with Integrated Frequency Converter

Type Designation	Part Numbers	Description			
<pre>< 3 Inlets TURBOVAC a1 a2 a3 i f1 f2 TURBOVAC a1 a2 a3 ix f1 f2 TURBOVAC a1 a2 a3 iC f1 f2 a1 = 850 or 950 or 1350 or 1450, a2=10to 1000, a3 = 1 to 500 (Indices a2 and a3 optional) f1 = 100 to 250 f2 = ISO-K or ISO-F or CF</pre>	8xxxxxVxxxxy x= 0 to 9 y = blank or U	a1 = Pumping speed (first Inlet) a2 = Pumping speed (second Inlet) a3 = Pumping speed (third Inlet) f1 = High Vacuum flange f2 = Flange type i = Communication electronic Frontend or Frontend Anybus iX = Communication electronic Extension box U = Upside Down iC / C = Cartridge - Housing for Customer Application m = Customer-Variants Multi-Inlet			
> 3 Inlets TURBOVAC numeral m i TURBOVAC numeral m iC	8xxxxxVxxxxy				
numeral = quad, penta, hexa,	x= 0 to 9				
hepta, octa, nona, deca (according to the number of inlets) m = 1 to 99	y = blank or C				

The object of the declaration described above is in conformity with relevant statutory requirements:

Supply of Machinery (Safety) Regulations 2008 The objectives of the Electrical Equipment (Safety) Regulations 2016 are governed by Annex 1 1.5.1 of this regulation.
Electromagnetic Compatibility Regulations 2016 Class B Emissions, Basic Industrial Immunity
Restriction of the Use of Certain Hazardous Substances in Electrical and Electronic Equipment Regulations 2012

Relevant designated standards or technical specifications are as follows:

EN 1012-2:1996 +A1:2009	Compressors and vacuum pumps. Safety requirements. Vacuum pumps			
EN 61010-1:2010/A1:2019	Safety requirements for electrical equipment for measurement, control and laboratory use. General requirements			
EN 61326-1:2013	Electrical equipment for measurement, control and laboratory use. EMC requirements. General requirements			

This declaration, based on the requirements of the listed Statutory Instruments and EN ISO/IEC 17050-1, covers all product serial numbers from this date on: 2021-06-14

You must retain the signed legal declaration for future reference This declaration becomes invalid if modifications are made to the product without prior agreement.

Signed for and on behalf of Leybold GmbH

Ian Keech – VP Engineering, Scientific Vacuum Division Burgess Hill

Axel Guddas – General Manager Cologne

ADDITIONAL LEGISLATION AND COMPLIANCE INFORMATION

RoHS (EU, UK): Material Exemption Information

This product is compliant with the following Annex III Exemptions:

- 6(a) Lead as an alloying element in steel for machining purposes and in galvanised steel containing up to 0.35 % lead by weight
- 6(b) Lead as an alloying element in aluminium containing up to 0.4% by weight
- 6(c) Copper alloy containing up to 4% lead by weight

REACH (EU, UK)

This product is a complex article which is not designed for intentional substance release. To the best of our knowledge the materials used comply with the requirements of REACH. The product manual provides information and instruction to ensure the safe storage, use, maintenance and disposal of the product including any substance based requirements.

Article 33.1 Declaration (EU, UK)

This product contains Candidate List Substances of Very High Concern above 0.1%ww by article as clarified under the 2015 European Court of Justice ruling in case C-106/14.

- Lead (Pb)
 - This substance is present in certain steel / aluminium / brass components.

Additional Applicable Requirements

The product is in scope for and complies with the requirements of the following:

2012/19/EU	Directive on waste electrical and electronic equipment (WEEE)
Product is certified to CSA-C22.2 No.61010-1-12	Safety requirements for electrical equipment for measurement, control and laboratory use – Part 1: General requirements
Product is certified to UL61010-1 3 rd Edition	Safety requirements for electrical equipment for measurement, control and laboratory use – Part 1: General requirements

材料成分声明

China Material Content Declaration

表示该有害物质在该部件的所有均质材料中的含量低于 GB/T 26572 标准规定的限量要求。 Indicates that the hazardous substance contained in all of the homogeneous materials for this part is below the limit requirement in GB/T 26572.

	有害物质 Hazardous Substances							
部件名称 Part name	铅 Lead (Pb)	汞 Mercury (Hg)	鎘 Cadmium (Cd)	六价铬 Hexavalent Chromium (Cr VI)	多溴联苯 Polybrominated biphenyls (PBB)	多溴二苯醚 Polybrominated diphenyl ethers (PBDE)		
铸铝及铝合金制品 Aluminium alloys	х	0	0	0	0	0		
钢合金制品 Steel alloys	х	0	0	0	0	0		
铜管管件 Brass pipe fitting	Х	0	0	0	0	0		

O:表示该有害物质在该部件的所有均质材料中的含量低于 GB/T 26572 标准规定的限量要求。

O: Indicates that the hazardous substance contained in all of the homogeneous materials for this part is below the limit requirement in GB/T 26572.

X: 表示该有害物质在该部件的至少一种均质材料中的含量超出 GB/T26572 标准规定的限量要求。 X: Indicates that the hazardous substance contained in at least one of the homogeneous materials used for this part is above the limit requirement of GB/T26572.



Pioneering products. Passionately applied.

Leybold GmbH Bonner Strasse 498 50968 Cologne GERMANY T: +49-(0)221-347-0 info@leybold.com www.leybold.com